

## Transmitting the data

Take a reading **daily** unless advised otherwise by your healthcare provider. The LED will turn **RED** at **midnight** and then turn **GREEN** once a measurement has been successfully transmitted.



Measurement Needed



Measurement Successful

7

## Power your Gateway

Plug your **Gateway** into a power outlet with the provided power cord and wait until the LED on the Gateway turns **RED**.



1



For more information about your device, use your phone to scan the QR code above or visit our support site at [tenovi.com/14](https://tenovi.com/14)

# tenovi


© 2025 Tenovi Co.

All rights reserved. Republication, duplication or modification in whole or in part is prohibited without prior written permission from Tenovi. All trademarks are owned by or licensed to Tenovi, Co, unless otherwise noted.

Revision 01.05.25

## Install batteries and setup


Install batteries and remove the protective film from the flat end of the device. Turn on the device by holding down the **power button** for **three seconds**. Volume can be adjusted on the side.

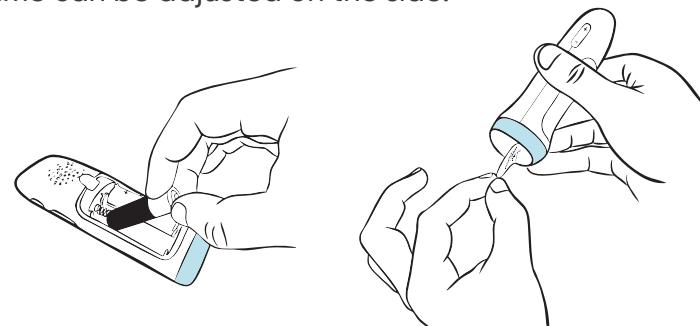

2

## Position your body


**Lay back** in a comfortable position on your bed with pillows behind your back. Cover the flat end of the device with a thin layer of Gel.

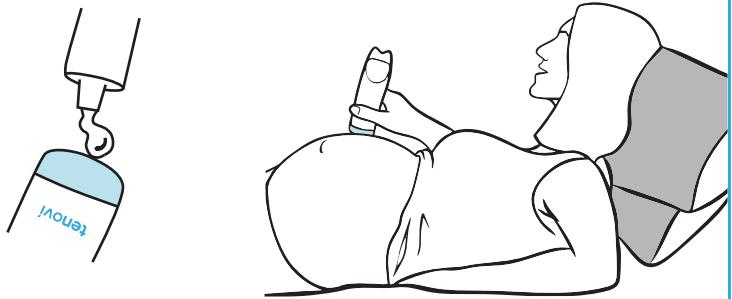

3


## Finding the baby's heart

Babies change positions. **Adjust the angle** until you hear the baby's heartbeat. If you aren't getting a good signal, **move to the next dot on the diagram** repeating the same hand motion until you hear the heartbeat loud and clear for a minimum of 6 seconds.

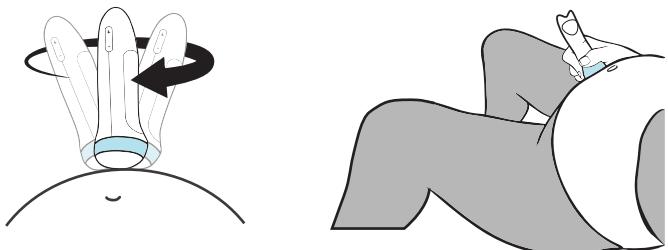


5


## Place the device on your belly



16 - 24 Weeks



24 - 32 Weeks



32 - 40 Weeks

Press the **flat end of the device** on the skin on the blue dot in the diagram. Apply enough pressure so the device maintains **full contact** with the belly.

4

## Successful Measurement

After getting a **clear audio signal**, the baby's heartrate will be **transmitted to the Gateway and sent to your provider**. The Gateway will beep twice for your first reading, once for each following reading, and three extra times on the 24th reading. Turn the device off and back on to transmit more readings to your Gateway.



6